



Handheld digital IR CAMERA

The Contour M offers significantly higher infrared sensitivity than conventional cameras, achieved through optimized photodiode surface area and depth, along with proprietary microlenses on each diode for enhanced light capture and focus. This design delivers a higher saturation signal, reduced smear and noise, and improved quantum efficiency in low-light conditions. Its automatic contrast control system boosts contrast up to 20 times, ensuring optimal observation across a wide range of illumination settings.



APPLICATIONS:

- Location and alignment of Nd:YAG Yb:YAG, Yb:KGW, Ti:Sapphire and other IR lasers
- Identification of stray IR reflections
- Observation of GaAs laser diodes, IR LED's, dye and other IR-sources
- Forensic analysis on inks, pigments

MAIN FEATURES:

- Built-in 4" LCD screen
- Operates up to 1900 nm
- High contrast and sensitivity(-70dB)
- USB-C Video Output for PC Capture and Recording
- Compatible with C-mount lenses
- Detects pulsed and continuous wave (CW) light
- Hands-Free Operation
- 9 hours continuous working

RoHs
CE


TECHNICAL INFORMATION

	MODEL (1X)	MODEL (2X)
Spectral sensitivity	400-1900 nm	
Power densities for effective viewing:	5 mW/cm ² at 1310nm 10 mW/cm ² at 1500nm 200 mW/cm ² at 1900nm	
Resolution (center)	30 Lp/mm	
Field of view	38°	19°
Magnification	1X	2X
Objective filter tread	F1.3/8mm M25.5x0.5	F1.4/16 mm M27x0.5
Objective thread	C-Mount 1"-32 UN	
Adjustable iris	Included	
Minimum object distance	0.1m to ∞ *	0.5m (0.15m) to ∞ *
Distortion of image	0.5%	
LCD Display	4" LCD	
Video interface	USB - C	
Battery	2 x 18650 batteries // Continuous operation for up to 9 hours	
Weight	0.64 kg	
Dimensions	134 x 90 x 42 mm	
Tripod thread	¼"-20 UNC	

* - MOD can be customized upon request


Lenses 1X (F1.3/8 mm) and 2X (F1.4/16 mm) are exchangeable.

NB! Use only for laser beam alignment and observation of the beam from surfaces and not for direct light pointing to sensor.



2x 18650 rechargeable batteries

To determine the battery polarity, check the markings located next to the battery insertion slots.






irvi infrared viewers



Power density

Threshold power density dependence on wavelength. The threshold power density is defined by measuring a laser beam spot on a paper, which exhibits 20% of the overall brightness (calculated as $255 \times 20\% = 51$), in contrast to the background. The measurements were taken with the camera positioned 1.15 meters away from the piece of paper.



Brightness levels

Normalised brightness dependence on power difference from the minimum value. The power level of 0 signifies the theoretical minimal value at which the laser beam spot becomes observable on a piece of paper. It's worth noting that the camera exhibits lower sensitivity to laser light at 1450nm compared to 1550nm or even 1900nm.


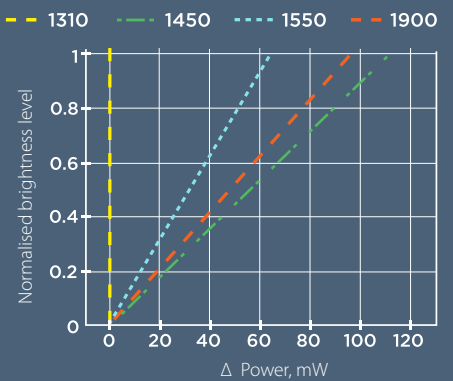


Approximate minimum power density required to observe an infrared laser source from a distance of one meter:

20 $\mu\text{W}/\text{cm}^2$
for a 1060 nm


500 $\mu\text{W}/\text{cm}^2$
for a 1300 nm

Neutral density filters transmission curves




For optional use at higher than about 200 mW lasers (@1064nm) (does vary with wavelength, refer to spectral sensitivity curve), you may consider using following filters to avoid sensor overfilling („light flooding“) issues and still ensure high visibility of your surroundings as the filter maintains high transmittance in the visible region compared to regular neutral density filters.

BP 39 Filter Internal Transmittance 1 mm Thickness



80 LP760 Filter



BP 212 Filter Internal Transmittance 2 mm Thickness

